

KETERANGAN PEMBELIAN TEMPATAN - JKP KEMENTAH

RUJUKAN SEBUTHARGA : MINDEF/DFA/FY2026/NAU/DEN/LP/1006

TARIKH TUTUP SEBUTHARGA : 27 - 8 - 2026 (KHAMIS, 08:00 PAGI)

PETI PENERIMAAN SEBUTHARGA : BOX (4)

ALAMAT BARU: BANGUNAN ARKIB, ARAS BAWAH, KEMENTERIAN PERTAHANAN,
BOLKIAH GARISON

NAMA SYARIKAT : _____

CAP SYARIKAT DAN TANDATANGAN : _____

TEL PEMBEKAL : _____ FAX PEMBEKAL : _____

E-MAIL PEMBEKAL : _____

VENDOR ID PEMBEKAL : _____

BIL	KETERANGAN BARANG	KTI	HARGA SATU	HARGA SEMUA	TEMPOH SAH HARGA (MINIMUM 180 HARI)	TEMPOH PENGHANTARAN	BUATAN NEGERI	LAIN-LAIN HAL
1	<u>PEMBELIAN PERALATAN DAN KELEGGAPAN PERGIGIAN (DENTAL EQUIPMENT)</u> OUTDOOR WATER FILTER (Sila rujuk spesifikasi di sertakan)	06 UNIT						
PERHATIAN: Perkara-perkara yang perlu (mandatori) di hadapkan sebelum tarikh tutup sebutharga : ☒ Katalog & Spesifikasi Teknikal mesti di sertakan untuk penilaian. ☐ Contoh Jika di dapati gagal, sebutharga tersebut tidak akan di pertimbangkan. PERINGATAN: Tidak dibenarkan menggunakan katalog Jabatanarah ini.								

10/8

JUMLAH SEMUA HARGA YANG DI TAWARKAN - ANGKA B\$ _____ DAN PERKATAAN: _____

Dental Maintenance Equipment	
Demand Reference	DSE/07/26/06
Description	Outdoor Water Filter
Quantity Required	6 units

Ser	Technical Data & Dimensional		Offer
	Item	Specification	
(a)	(b)	(c)	(d)
Essential			
1	General	The outdoor water filter is for the treatment of incoming water supply. The system shall be designed to improve water quality by removing suspended solids, sediment, chlorine, unpleasant odor and other physical impurities before the water enters the building's internal plumbing system.	
2	Technical data	Type: Outdoor Multi-media water filtration system Installation: Point-of-Entry (POE) System Filter Tank Size: Minimum 10 inches diameter x 44 inches height Filter Media: Multi-layer media comprising Silica Sand, Activated Carbon and other suitable filtration media Filtration Rating: 30-50 micron or finer Water Treatment: Removal of sediment, rust, suspended particles, chlorine, color, taste and odor Tank Material: Corrosion-resistant FRP or equipment heavy-duty pressure vessel Valve: Heavy duty automatic or manual multi-port control valve Working Pressure: Suitable for normal municipal water supply Connection: Compatible with existing plumbing system Operating Temperature: Suitable for tropical climate	
3	Features	Automatic Backwash Multi-stage filtration using high-quality filtration media Effective removal of sediment, rust particles and suspended solids Activated carbon filtration for reduction of chlorine, unpleasant taste and odor Corrosion resistant filter vessel suitable for outdoor installation Durable construction requiring minimal maintenance Easy servicing and replacement of filter media Reliable operation with minimal pressure loss Suitable for continuous daily operation Complete with inlet, outlet, bypass piping and necessary	



		accessories Designed for long service life under tropical environmental conditions	
	Requirements	The Contractor shall provide the following as part of the tender: Supply • Supply one (1) complete Outdoor Water Filtration System for Berakas Dental Centre • Supply one (1) complete Outdoor Water Filtration System for Lumut Dental Centre • Supply one (1) complete Outdoor Water Filtration System for Tutong Dental Centre • Supply one (1) complete Outdoor Water Filtration System for Penanjong Dental Centre • Supply one (1) complete Outdoor Water Filtration System for Muara Dental Centre • Supply one (1) complete Outdoor Water Filtration System for Rimba Dental Centre Installation • Complete installation including all piping, fittings, valves, connectors and commissioning. • Integration with the existing water supply system • Testing and commissioning to ensure satisfactory operation Extra Job Required • Build shelter to protect the water filter electronic system (Automatic flushing) for Rimba Dental Centre and Berakas Dental Centre Warranty • Minimum three (3) years warranty covering manufacturing defects. • Warranty shall include the filter tank, control valve and filtration components. • Replacement of defective parts during the warranty period shall be at no additional cost. Preventive Maintenance The Contractor shall provide: • Preventive maintenance for a minimum period of three (3) years. • Maintenance visits of every six (6) months. • Inspection, servicing, cleaning and performance checks during each maintenance visit. • Replacement of consumable filtration media where required (if included in the maintenance	



		package).	
		After-Sales Support The contractor shall provide: • Technical support during office hours. • Emergency breakdown support. • Availability of spare parts throughout the warranty period. • Qualified technicians for maintenance and repair services.	
Installation and Support			
4	Approved Agent Status	It is essential that the contractor/ Supplier submit a letter from the manufacturer stating that they: • Manufacturers authorized the supplier of the equipment • Are authorized by the manufacturer to deliver; test and commission their equipment	
5	Warranty	It is essential that the manufacturer provided a minimum of 1 year warranty support (parts and labor) from the date of acceptance into service	
Desirable			
6	Preferred Model/ Brand & country Origin of the manufacturer	Outdoor Water Filter Blondal 1054 (Auto) or Equivalent	



*Important Notice


This specification annex form must complete and attached with the quotation tenders provided.

Company / Supplier Chop & Signature

.....

Dental Services RBAF Demand Catalogue Reference

Appendix 8-1

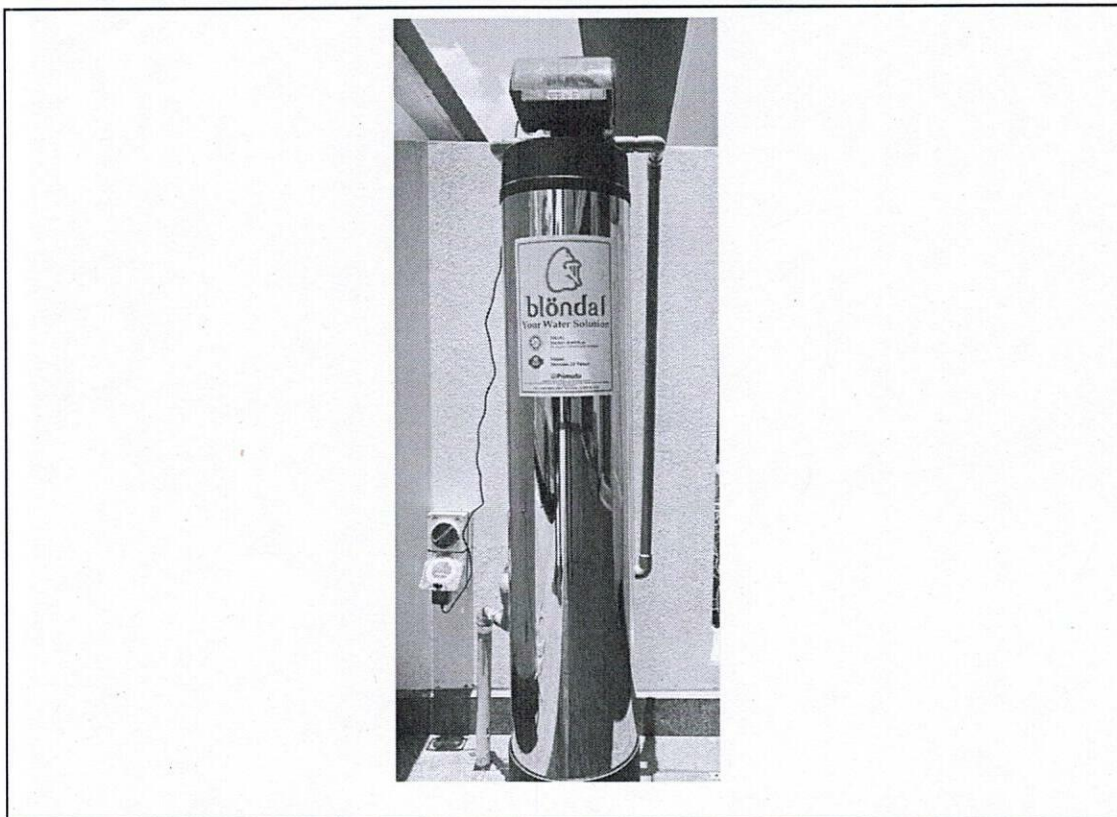

Dental Maintenance Equipment	
Dental Services RBAF Demand Reference	DSE/07/26/06
Descriptions	Outdoor Water Filter
Quantity Required	6 Units
Preferred Model/Brand & Country Origin of the Manufacturer	Outdoor Water Filter Blöndal 1054 (Auto) or Equivalent
Submitting Catalogue/Brochures	The Supplier must submit the Catalogue/brochures completely for the offered item.

