

KETERANGAN PEMBELIAN TEMPATAN - JKP KEMANTAN

RUJUKAN SEBUTHARGA : MINDEF/DFA/FY2026/NAU/DEN/LP/1013

TARIKH TUTUP SEBUTHARGA : 15 - 10 - 2026 (KHAMIS, 08:00 PAGI)

PETI PENERIMAAN SEBUTHARGA : BOX (3)

ALAMAT BARU: BANGUNAN ARKIB, ARAS BAWAH, KEMENTERIAN PERTAHANAN,
BOLKIAH GARISON

NAMA SYARIKAT : _____

CAP SYARIKAT DAN TANDATANGAN : _____

TEL PEMBEKAL : _____ FAX PEMBEKAL : _____

E-MAIL PEMBEKAL : _____

VENDOR ID PEMBEKAL : _____

BIL	KETERANGAN BARANG	KTI	HARGA SATU	HARGA SEMUA	TEMPOH SAH HARGA (MINIMUM 180 HARI)	TEMPOH PENGHANTARAN	BUATAN NEGERI	LAIN-LAIN HAL
1	<u>PEMBELIAN PERALATAN DAN KELEGGAPAN PERGIGIAN (DENTAL EQUIPMENT)</u> DENTAL SURGICAL UNIT (Sila rujuk spesifikasi di sertakan)	02 UNITS						
PERHATIAN: Perkara-perkara yang perlu (mandatori) di hadapkan sebelum tarikh tutup sebutharga : ☒ Katalog & Spesifikasi Teknikal mesti di sertakan untuk penilaian. ☐ Contoh Jika di dapati gagal, sebutharga tersebut tidak akan di pertimbangkan. PERINGATAN: Tidak dibenarkan menggunakan katalog Jabatanarah ini.								

JUMLAH SEMUA HARGA YANG DI TAWARKAN - ANGKA B\$ _____ DAN PERKATAAN: _____

Dental Surgical Equipment	
Demand Reference	DSE/06/26/05
Description	Dental Surgical unit
Quantity Required	2 units

Ser	Technical Data & Dimensional		Offer
	Item	Specification	
(a)	(b)	(c)	(d)
Essential			
1	General	The dental surgical unit system is a premium surgical motor system used for carrying out minor oral surgery procedures on patient. It contains small surgical micro-motors that delivers high torque at the instrument with precise auto-calibration and smart, low-vibration performance to enable the Oral Surgeon to cut teeth and bone efficiently and effectively whilst maintaining patient safety. Dental Services RBAF conducts on average 500 surgical procedures in-house a year on patients, minimizing the need for specialist referral for oral surgery to the ministry of health.	
2	Technical data	Power Supply	100V - 240V AC
		Input Frequency	50/60 Hz
		Pump performance	0 - 110 ml / min
		Implant systems	4 - 10 Programs
		Treatment steps	Max.10
		Pumping Power	0 - 4
		Torque	5-80 Ncm
		Motor Speed	200~40,000 min-1
		Light Power(LED Micromotor)	over 32,000 LUX
3	Features	High resolution LCD colour display. Surgical programme with up to 10 customisable treatment steps. Fast, intuitive programming via touch buttons. Powerful, ultra-lightweight S600 LED surgical motor with maximum torque adjustable up to 5.5 Ncm. SMARTdrive function for extra- smooth running. Accurately adjustable torque shown on the display for safe implantation without exceeding the maximum permissible torque value Safe hygiene concept that meets the very highest standards. Freely programmable workflows make work easier Visual representation of all program steps – rapid	



		recognition of activity Indication – dependent limitation of parameters – rapid adjustment ‘Free application’ activity – all parameters freely adjustable Navigation during treatment using foot control LED optic surgical motor/unit from KaVo: • One-touch auto-calibration – ensures precise speed and torque for maximum safety. Automatic process. • Easy to use interface – symbolic references, colour display. Accurate display of adjusted max. torque and motor speed. • Hygienic design – smooth surface, easy to clean. Thermo-disinfectable and sterilisable motor and motor tube. • Guaranteed precision – one of the world’s lightest and smallest surgical micromotors. Smooth running with low vibration. • High performance – 80 Ncm torque at the handpiece. SMARTdrive technology gives high performance and minimal vibration from the start. Six customisable parameters: • Treatment steps (max. 10) • Change of contra-angle transmission ratio • Max speed • Max torque • Pumping power (0 – 4) • Motor Forward/Reverse	
	Accessories to be included	✓ INTRA LUX S600 LED – 2 units (1 extra) ✓ SURGmatic Hand piece S11 L (1:1) – 2 units ✓ SURGmatic S15 L Pro Contra-Angle (1:5) – 2 units ✓ Multifunctional foot control (cable length 2.5m) ✓ Starter tube set (5 pieces) ✓ Irrigation bracket ✓ Motor Tubing for S600 LED ✓ Motor and instrument holder ✓ Integrated peristaltic pump ✓ Power Supply	



Installation and Support			
4	Approved Agent Status	It is essential that the contractor/ Supplier submit a letter from the manufacturer stating that they: - Manufacturers authorized the supplier of the equipment - Are authorized by the manufacturer to install; test and commission their equipment	
5	Warranty	It is essential that the manufacturer provided a minimum of 1 year warranty support (parts and labor) from the date of acceptance into service	
Desirable			
6	Preferred Model/ Brand & country Origin of the manufacturer	EXPERTsurg LUX Surgical Unit or Equivalent	

*Important Notice

This specification annex form must complete and attached with the quotation tenders provided.




Company / Supplier Chop & Signature

.....

Dental Services RBAF Demand Catalogue Reference

Appendix 8-1

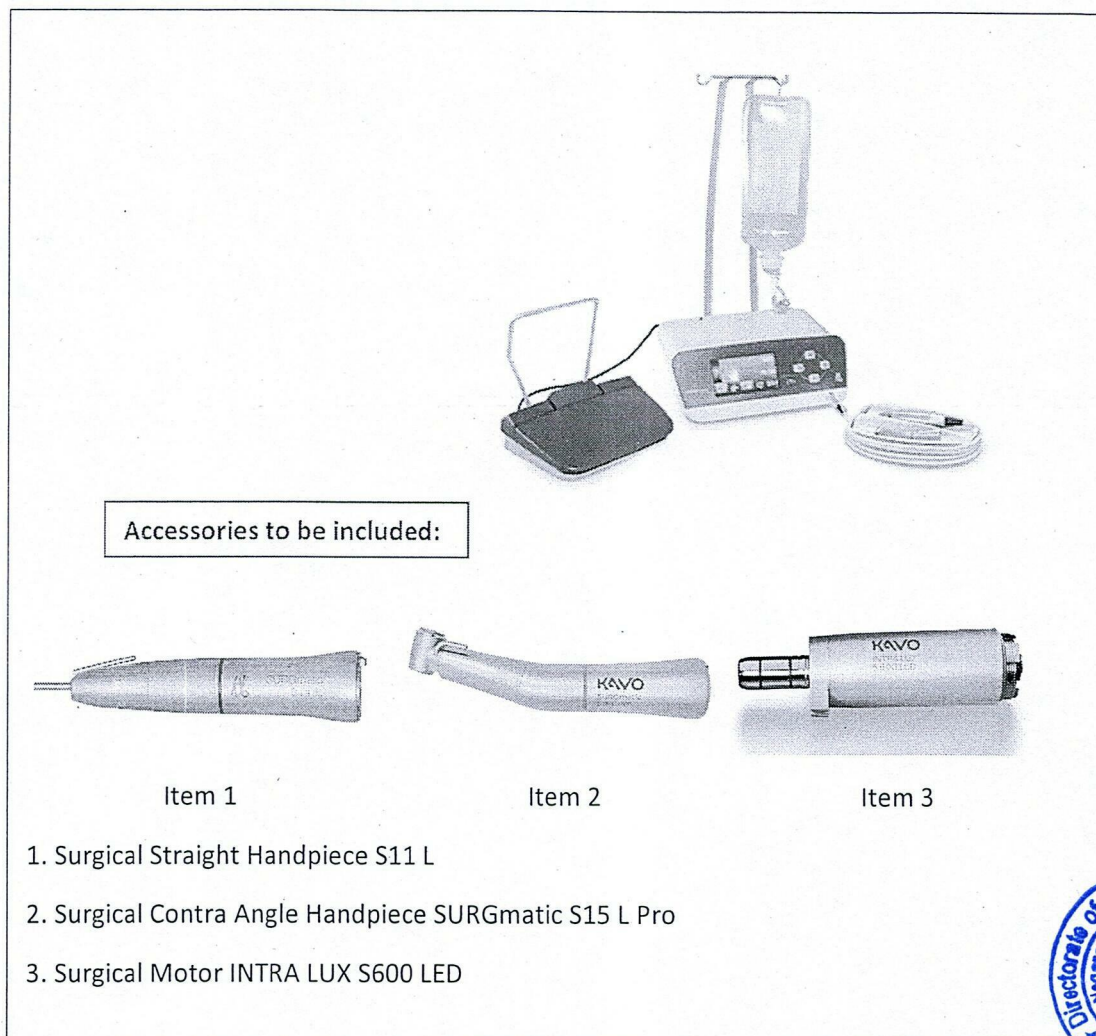

Dental Surgical Equipment	
Dental Services RBAF Demand Reference	DSE/06/26/05
Descriptions	Dental Surgical unit
Quantity Required	2 Units
Preferred Model/Brand & Country Origin of the Manufacturer	EXPERTsurg Lux Surgical Unit or Equivalent
Submitting Catalogue/Brochures	The Supplier must submit the Catalogue/brochures completely for the offered item.